

Opus™360 Nasal Pillows Mask Patient Instructions for Use

The Opus™360 Nasal Pillows Mask is intended to be used by individuals who have been diagnosed as apnoeic by a physician requiring CPAP or Bi-level therapy for ventilation. The Opus™360 mask is intended for Single Patient Adult Use. This mask is designed for use with the Fisher & Paykel AutoSet or the Fisher & Paykel AutoSet Pro CPAP or Bi-level Therapy System. The mask should be used as directed in the user manual. The mask is intended for use with the Opus™360 Nasal Pillows Mask. The mask is not to be used for any other purpose. The mask is not to be used for any other purpose. The mask is not to be used for any other purpose.

Operating Instructions:

- The operating pressure range of the mask is 3 to 21 cm H₂O.
- The operating temperature range of the mask is 14°C to 40°C (57°F to 104°F).
- Before use, inspect the mask for damage.
- Inspect for damage: If there is any visible deterioration (tearing, rips or tears) or any other damage to the mask, do not use it.
- Inspect the vents: Do not use if blocked.
- Check the fit: The mask should fit snugly around the bridge of the nose.

Warnings & Cautions:



- This mask should be used only with CPAP or Bi-level equipment recommended by your physician or respiratory therapist. A mask should not be used unless the CPAP or Bi-level machine is turned on and operating properly.
- Do not use the mask while driving or operating machinery.
- Do not use the mask if you have a condition that could be worsened by CPAP or Bi-level therapy.
- Do not use the mask if you have a condition that could be worsened by CPAP or Bi-level therapy.

Fit the Mask:

- Place the mask over the nose and mouth.
- Adjust the headgear to fit comfortably.
- Adjust the headgear straps to fit comfortably.
- Adjust the headgear straps to fit comfortably.
- Adjust the headgear straps to fit comfortably.

Mask Assembly:

- Remove the mask from the box.
- Remove the mask from the box.
- Remove the mask from the box.
- Remove the mask from the box.
- Remove the mask from the box.

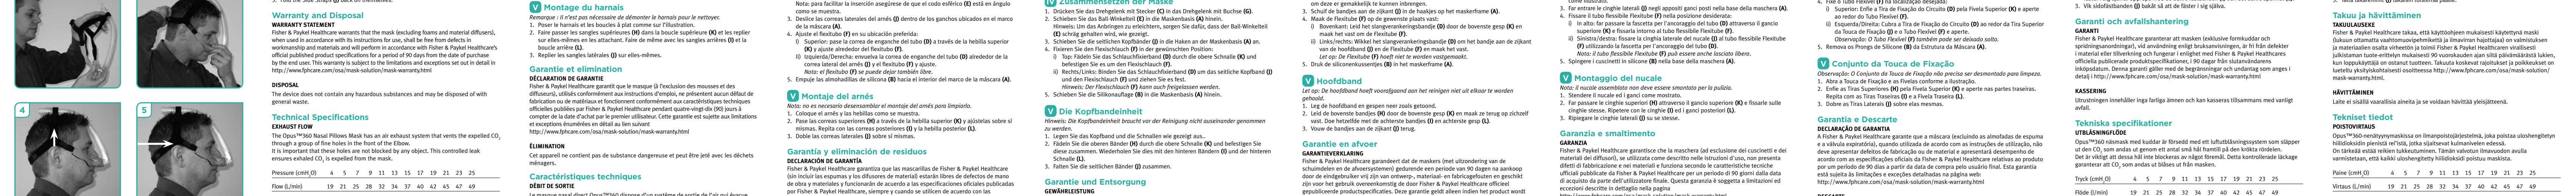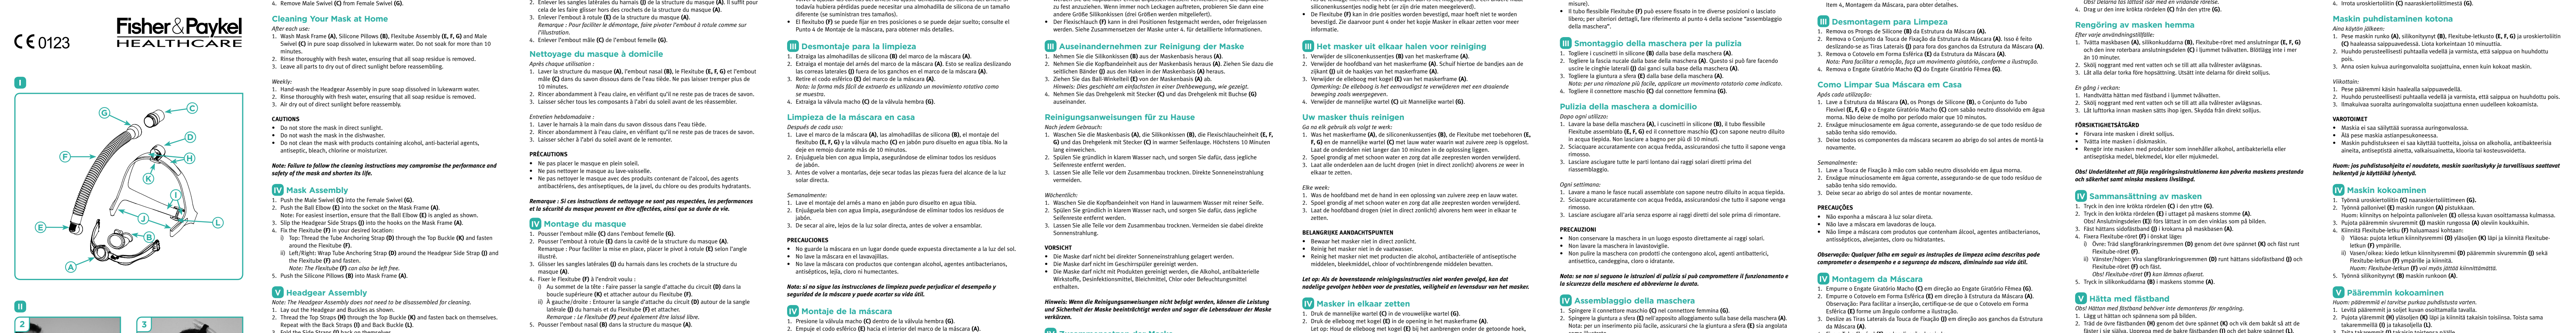

Technical Specifications:

Resistance to Flow:

Flow (L/min)	Pressure (cmH ₂ O)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

Resonance to Flow:

Pressure (cmH ₂ O)	Flow (L/min)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

Resistance to Flow:

Flow (L/min)	Pressure (cmH ₂ O)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

Resonance to Flow:

Pressure (cmH ₂ O)	Flow (L/min)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

Resistance to Flow:

Flow (L/min)	Pressure (cmH ₂ O)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

Resonance to Flow:

Pressure (cmH ₂ O)	Flow (L/min)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

Resistance to Flow:

Flow (L/min)	Pressure (cmH ₂ O)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

Resonance to Flow:

Pressure (cmH ₂ O)	Flow (L/min)
4	5
7	9
11	13
15	17
19	21
23	25

Mask Dead Space:

Pressure (cmH ₂ O)	Flow (L/min)
19	21
23	25
27	29
31	33
35	37
39	41
43	45
47	49

